

**Slovak University of Technology in Bratislava
Institute of Information Engineering, Automation, and Mathematics**

PROCEEDINGS

17th International Conference on Process Control 2009

Hotel Baník, Štrbské Pleso, Slovakia, June 9 – 12, 2009

ISBN 978-80-227-3081-5

<http://www.kirp.chtf.stuba.sk/pc09>

Editors: M. Fikar and M. Kvasnica

Adámek, M., Matýsek, M., Kodriková, K.: Modelling and Design of Microflow Sensors Based on Measuring of Temperature, Editors: Fikar, M., Kvasnica, M., In *Proceedings of the 17th International Conference on Process Control '09*, Štrbské Pleso, Slovakia, 263–267, 2009.

Full paper online: <http://www.kirp.chtf.stuba.sk/pc09/data/abstracts/102.html>

MODELLING AND DESIGN OF MICROFLOW SENSORS BASED ON MEASURING OF TEMPERATURE

M. Adámek*, M. Matýsek, and K. Kodriková***

* *Faculty of Applied Informatics, Thomas Bata University in Zlin*
fax : +420 576 032 716 and e-mail : adamek@fai.utb.cz

** *Faculty of Applied Informatics, Thomas Bata University in Zlin*
fax : +420 576 032 716 and e-mail : matysek@fai.utb.cz

Abstract: This article describes modelling and measurement of tiny liquid flows of the order of microlitres through millilitres per minute. The measurement of mentioned flow range is becoming more and more important for a lot of applications in the life science, analysis, biotechnologies, synthesis (of e.g. pharmaceuticals) and nanotechnology markets. Accompanying demands to flow sensors suited for this low flow range are an extremely small internal volume, the use of for instance PEEK and fused silica as wetted material for the flow sensor tube (instead of stainless steel), and a modular set-up of the instruments, so they can be easily exchanged and adapted to a new need.

Keywords: sensor, flow, model, measuring.

1 INTRODUCTION

The modelling of microsystems requires appropriate compact or macro models for microdevices. In general, it is difficult or almost impossible to obtain closed form analytical models for microdevices. Thus, models are obtained by a simplification of the full physical model. The compact models allow for fast system level simulation of the microsystem. However, the accuracy of such a model can be questionable because of the simplifications made during the model development phase. Model accuracy and simplicity are important for the design of complex systems. Microflow sensor modelling has been examined by several authors (Hardy 1998) These approaches have used a solution of the partial differential equations (PDEs) for the coupled fluid/thermal problem. The work of (Kolomazník 2000) employs equivalent circuit descriptions that are solved in SPICE whereas (Lammerink1993) solve the PDEs using the finite-element and the finite-difference methods, respectively. However, none of these methods provide a simple and accurate macromodel for the flow sensor.

In this paper is presented modelling approach for microflow sensor and design of microflow sensor.

2 DESCRIPTION OF PRINCIPLES OF FLOW SENSOR

This work is focused on the modelling of a thermal method for mass flow determination of flowing media. A basic principle of a design flowmeter is shown in Figure1. This flowmeter type is called as time – of – flight sensor. The time – of – flight sensor consists of a heater and one or more temperature sensors downstream. The heater is activated by current pulses. The transport of the generated heat is a combination of diffusion and forced convection. The resulting temperature field can be detected by temperature sensors located downstream. The sensor output is the time difference between the starting point of the generated heat pulse and the point in time at which a maximum temperature at the downstream sensor is reached. The time – of – flight sensors have the same limitations as the intrusive type of calorimetric sensors: corrosion, erosion and leakage. Since the signal processing needs a short while to measure the time difference, this sensor type is not suitable for dynamic measurement.

The transport of the heat generated in line source through a fluid is governed by the energy equation

$$\frac{\partial T}{\partial t} + v \nabla T = \left(\frac{\lambda}{\rho c} \right) \nabla^2 T + \frac{q'}{\rho c} \quad (1)$$

where T is the temperature, c is the specific heat at the constant pressure, ρ is the density, v is the kinematic viscosity of the fluid, λ is the thermal conductivity and q' (in W m^{-3}) is the amount of heat per unit of volume and time. The analytical solution of this differential equation for a pulse signal with input strength q'_o (W m^{-1}) is given in (Webster 2000) as :

$$T(x, y, t) = \left(\frac{q'_o}{4\pi\lambda t} \right) \exp \left\{ -\frac{[(x - vt)^2]}{4at} \right\} \quad (2)$$

where a denotes the thermal diffusivity.

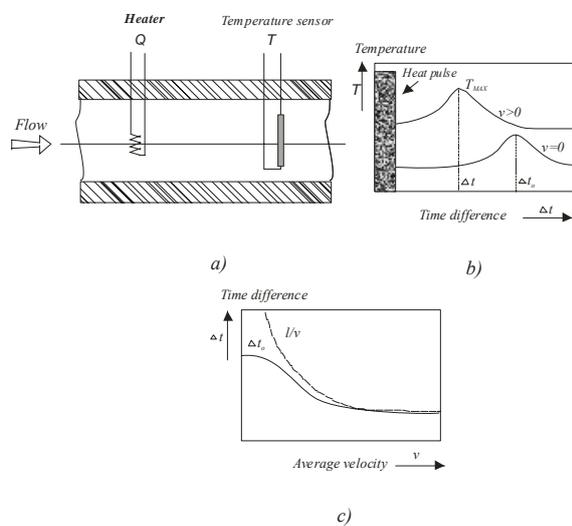


Fig. 1. Principles of the Time – of – flight sensor

The designed flowmeter is modified version of the time – of – flight sensor. In this case a temperature field is measured by semiconductor film located in top part of sensor tube. The temperature profile in semiconductor film depends on gas velocity. The heater is activated periodically; the period of the heat pulses generation can be different for different velocity size.

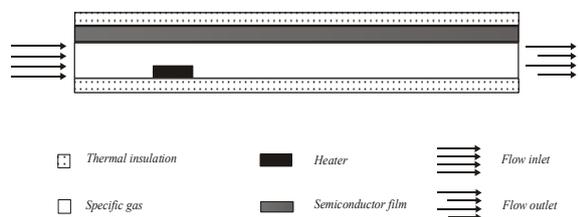


Fig. 2. Modified version of the time – of – Flight sensor

3 NUMERICAL MODEL

3.1 Basic Equations for $T(x,y)$

The simulated time – of – flight sensor is a multiphysics model, meaning that it involves more than one kind of physics. In this case, there are Navier-Stokes equations from fluid dynamics together with a heat transfer equation that is essentially a convection-diffusion equation. There are four unknown field variables: the velocity field components u and v , the pressure p and the temperature T . They all are inter-related through bidirectional multiphysics couplings.

The pure Navier-Stokes equations consist of a momentum balance (a vector equation) and a mass conservation. The equations are

$$\rho \frac{\partial u}{\partial t} + \rho(u \cdot \nabla)u = -\nabla p + \eta \nabla^2 u + F \quad (3)$$

$$\nabla \cdot u = 0 \quad (4)$$

where F is a volume force, ρ is the fluid density and v is the dynamic viscosity.

The heat equation is an energy conservation equation that only says that the change in energy is equal to the heat source minus the divergence of the diffusive heat flux

$$\rho c_p \frac{\partial T}{\partial t} + \nabla \cdot (-k \nabla T + \rho c_p T u) = Q \quad (5)$$

where c_p is the heat capacity of the fluid and ρ is fluid density as before. The expression within the brackets is the heat flux vector and Q represents a source term. The heat flux vector contains a diffusive and a convective term, where the latter is proportional to the velocity field u .

3.2 Modelling Results

The modelling approach uses a numerical solution of the PDEs for constructing the model. First a steady-state model is developed and this is then extended to include the dynamic behaviour. The sequence of steps is outlined below

- a numerical solution is obtained for $T(x, y)$ from equations (3), (4) and (5) for different values of the velocity u , the height of the fluid channel d and the sensor width l
- this solution yields discrete data points for T_1 , T_2 , and T_3 as a function of u , d and l
- the discrete data points can be used for study of dynamic behaviour of study sensor.

The PDEs can be solved by using a numerical solver, such as CFD-ACE+ (Hardy 1998). However, for circuit-level simulations a macromodel is required. The macromodel must be computationally efficient

and provide an accurate description of the temperature in semiconductor film. In the present work, the properties of the time – of – flight sensor were investigated using commercially available program FEMLAB. Femlab is an interactive environment for modeling and solving problems based on partial differential equations. This program applies the finite element method (FEM) for solving of the PDEs system.

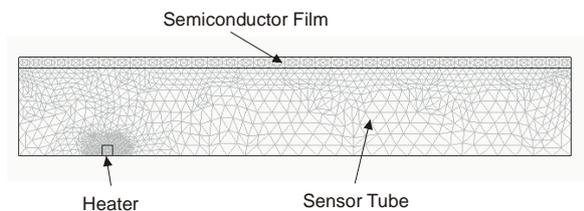


Fig. 3. Partial view of the computational grid for the basic configuration

The two dimensional configuration of the designed flowmeter in the present work can be seen in Figure 3. The heater generates heat in the time interval $<0,1>$ seconds. In the models the temperature change of the heater in time is shown in Figure 4.

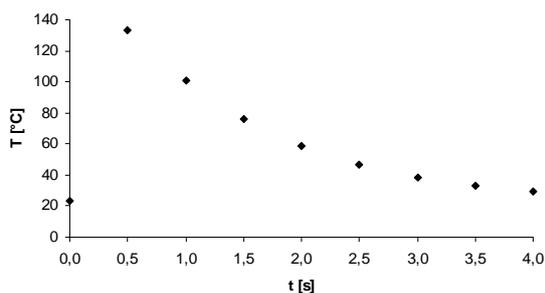


Fig. 4. Temperature change on the heater in time

In the sensor model the temperature of the heater has changed periodically, Figure 5.

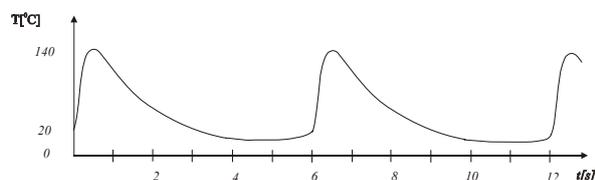


Fig. 5. The time path of the temperature of the heater

The properties of the modified time – of – flight sensor were simulated and verified for different flowing gases. The dependence of T_{MAX} on flow velocity v can be found in Figure. 7, 8, 9; the temperature T_{MAX} was measured in semiconductor film.

The temperature profiles in different time intervals in semiconductor film are shown in Figure 6.

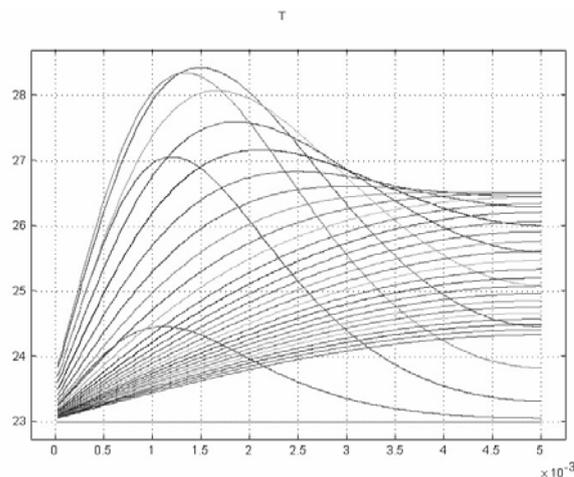


Fig. 6. The profile in semiconductor film (axis – x: distance, axis – y: temperature)

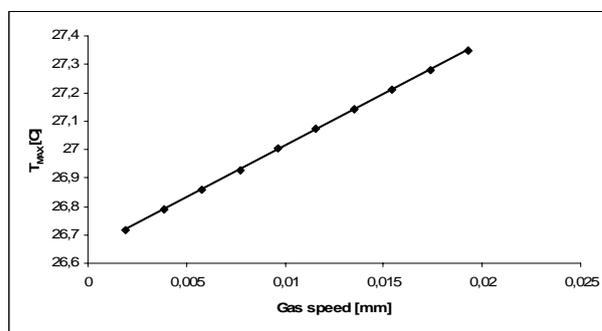


Fig.7. The dependence of T_{MAX} in semiconductor film on flow velocity v , gas–air, the diameter of the fluid channel $d = 1,2 \text{ mm}$

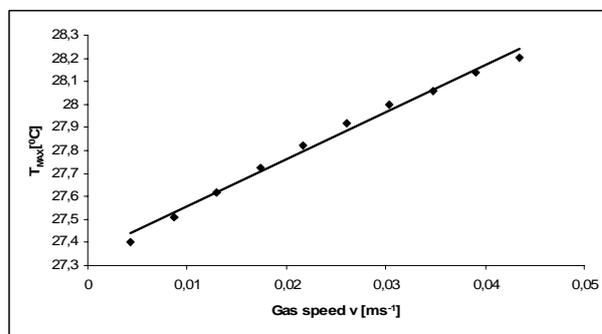


Fig.8. The dependence of T_{MAX} in semiconductor film on flow velocity v , gas – carbon dioxide, the diameter of the fluid channel $d = 0,8 \text{ mm}$

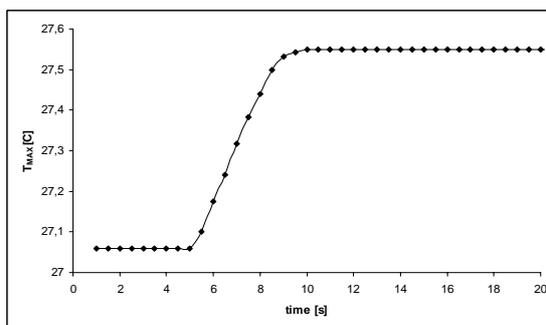


Fig.9. The time response of flow sensor: flow variation from 30 ml/hr to 100 ml/hr , the diameter of the fluid channel $d = 0,8 \text{ mm}$

4. EXPERIMENTAL SET-UP

The modified time-of-flight sensor consists of a heater placed on the pipe's floor and series of downstream sensors (semiconductor diodes) placed in the pipe's upper wall. The heater is activated for 1 second by a current pulse. The heat generated by the heater spreads with the flowing gas and leads into resistance changes on the diodes. The resistance change upon each diode is measured as a voltage change by an A/D converter. From the particular points along the pipe is set the wave's heat profile which is scanned for the temperature maximum position. The flow volume is proportional to the position shift in time. The scheme drawing is shown in Figure 10.

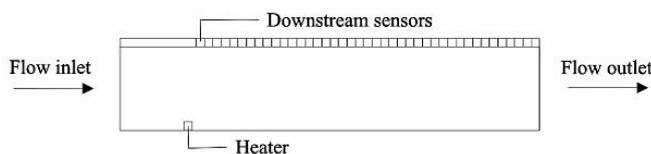


Fig.10. Experimental set-up of modified flow sensor

The heater is made from iron wire leaf, the semiconductor array is made of silicon. The whole pipe is put into a polystyrene casing to become thermally insulated from the ambient temperature conditions. The length of the pipe body has been set as 5mm.

4.1. Control Program

A program CONTROLWEB was used for visualisation.

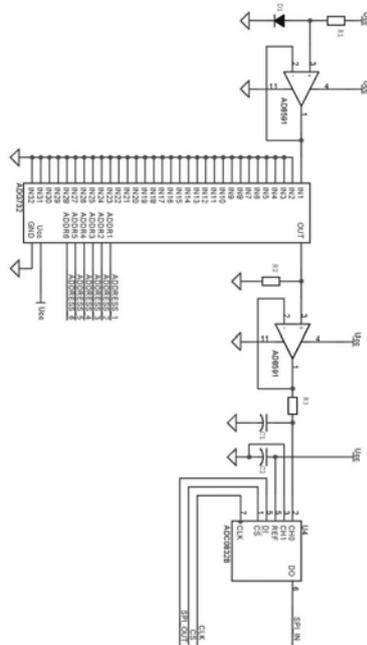


Fig.11. Block diagram of the modified sensor and saving of measuring data. A flow chart is presented in Figure 12. The resistance change upon each diode is measured as a voltage change by an A/D

converter. The voltage drops are measured in very short time periods, the period of measuring is 1ms. The voltage values are measured before bracing of the heating circuit and past disconnection of the heating circuit. By this philosophy is realized independence of the sensor output on the temperature of flow gas.

4.2. Experimental validation of modelling results

The validation of the finite-element/analytical model of the designed flowmeter was directly compared with experimental data. The peristaltic pump was used for the calibration of the modified time – of – flight sensor. The flow sensor was calibrated for air and CO₂. The measuring data can be seen in Figure 13.

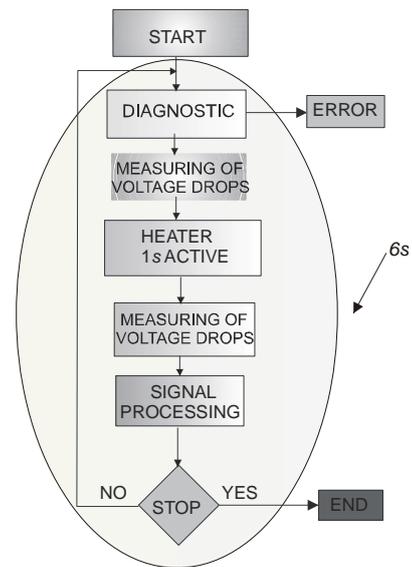


Fig.12. Flow chart

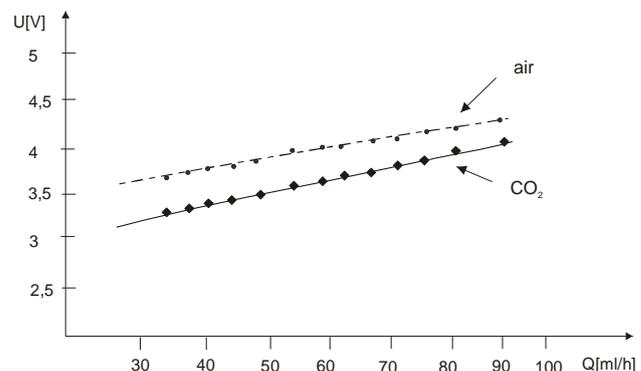


Fig.13. Static characteristic of modified sensor

5. CONCLUSION

This article describes properties of the modified time – of – flight sensor. The designed flowmeter has been used in a biochemical laboratory for study of reaction kinetic of a decomposition of sediments in waste water.

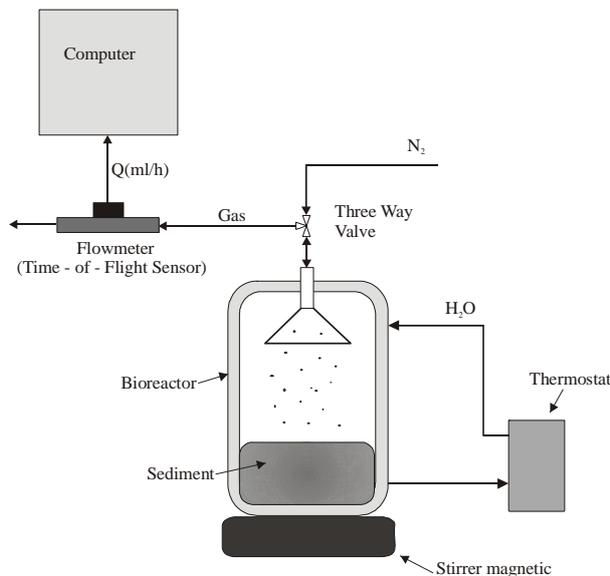


Fig. 14 The laboratory experiment set-up

The basic configuration is shown in Fig. 14. The decomposition reaction has three parts:

- degradation
- hydrolysis
- acetolysis.

The reaction kinetic of the studied decomposition reaction can be seen in Fig. 15.

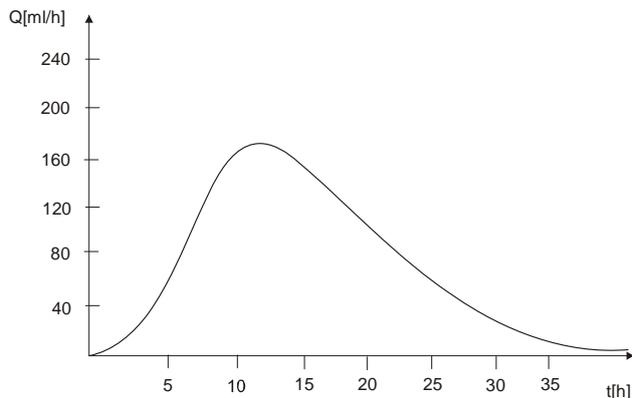


Fig. 15 The reaction kinetic of the decomposition reaction

ACKNOWLEDGMENT

The work has been supported by the Ministry of Education of the Czech Republic under grant MSM 708835102. This support is very gratefully acknowledged.

6. REFERENCES

Hardy, J., Hylton, O. (1999). *Flow measurement methods and applications*. Wiley –Interscience. USA.

Kolomazník, K., Taylor, M., Kupec, J. (2000). The valuable products from wastes. In.: *5th World Congress R'2000, Recovery, Recycling, Re-integrat.* Canada.p.5.

Lammerink, T., Niels, R., Elwenspoek, M. (1993). Micro – liquid flow sensor. *Sensors and actuators A*. Vol. 37/38, 45 – 50.

Lammerink, T., Dijkstra, F., Houkes, Z., Kuijk, J. (1995). Intelligent gas – mixture flow sensor. *Sensors and actuators A*. Vol. 46/47, 380 – 384.

Rasmussen, A., Zaghoul, M. (1999). The design and fabrication of microfluidic flow sensors. In.: *ISCAS-99*, 136- 139.

Webster, J. (1999). *Measurement, instrumentation and sensors*. USA, IEEE Press.